



ENDOSCOPE ROOM STERILE WATER TREATMENT EQUIPMENT

YS-RO-120L/H



YS-RO-120L/H series medical pure water treatment system utilizes single-stage RO system.



The equipment of this model is equipped with an external water tank.




The water quality produced by the equipment of this model conforms to WS 507-2016 Regulation for Cleaning and Disinfection Technique of Flexible Endoscope. The equipment is measured by conductivity meter, and the conductivity is $\leq 15\mu\text{s}/\text{cm}$ (25°C).




The equipment utilizes multi-sterilization process of membrane module + overflow ultraviolet + immersion sterilization module + advanced oxidation + terminal filtration to ensure the safety of customer water.



The preprocessing of the equipment of this model adopts multiple filtration methods: The first-class 20-inch thick wire winding, second-class canned coconut shell activated carbon/softened resin (with timing automatic washing), and third class 20-inch thick precision filtration, applicable to different areas of water quality, satisfy multiple customer needs.

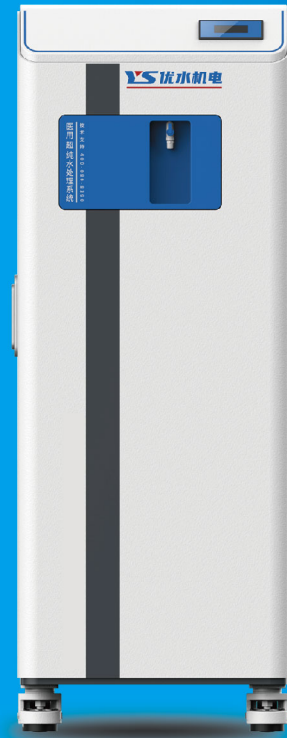

EQUIPMENT WORK FLOW CHART

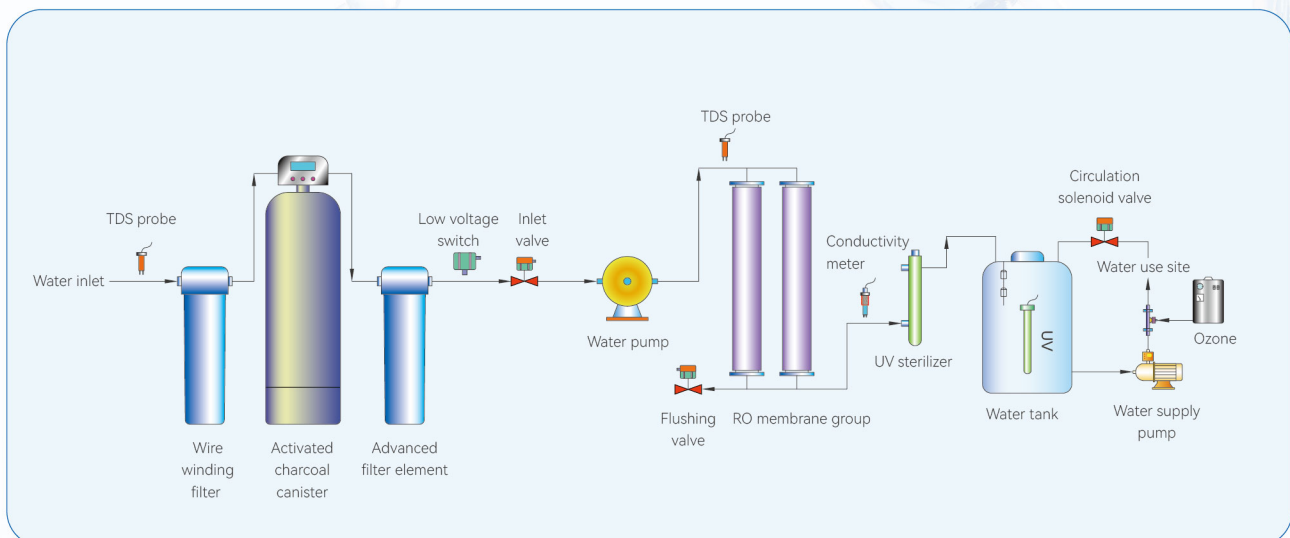

EQUIPMENT PARAMETER INFORMATION

EQUIPMENT PARAMETERS AND RELEVANT REQUIREMENTS	
Equipment model	YS-RO-120L/H
Water quality standards	WS 507-2016
Water output	120L/H
Quality of water production	
Microbial limit	≤10 CFU/100ml
Electrical conductivity μs/cm(25°C)	0.0050
Additional information	
Equipment size	54*56*148cm
Usage requirement	
Incoming water pressure	≥0.3MPa
Influent quality (TDS)	≤150ppm
Power supply	AC220V±10% 50HZ
Rated power	0.6kw
Scope of application	
Endoscope room disinfection and cleaning water	

EQUIPMENT CHARACTERISTICS AND ADVANTAGES



Artistic shape and appearance



Automatic start-stop



Renowned brand accessories at home and aboard



Easy installation and convenient replacement of consumables



Stable water production and quality



High water purity



Having independent intellectual property rights



IoT

YS-RO-150L/H



YS-RO-150L/H series medical pure water treatment system utilizes single-stage RO system.



The equipment of this model is equipped with an external water tank.




The water quality produced by the equipment of this model conforms to WS 507-2016 Regulation for Cleaning and Disinfection Technique of Flexible Endoscope. The equipment is measured by conductivity meter, and the conductivity is $\leq 15\mu\text{s}/\text{cm}$ (25°C).




The equipment utilizes multi-sterilization process of membrane module + overflow ultraviolet + immersion sterilization module + advanced oxidation + terminal filtration to ensure the safety of customer water.



The preprocessing of the equipment of this model adopts multiple filtration methods: The first-class 20-inch thick wire winding, second-class canned coconut shell activated carbon/softened resin (with timing automatic washing), and third class 20-inch thick precision filtration, applicable to different areas of water quality, satisfy multiple customer needs.

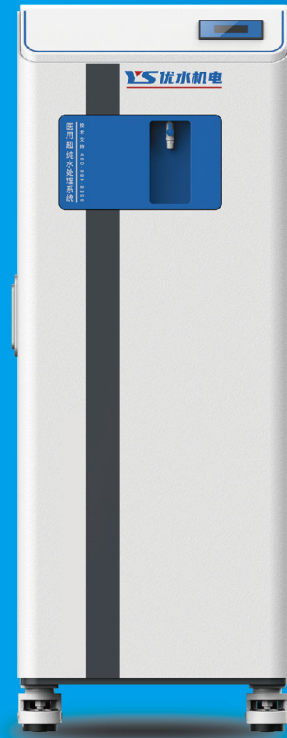

EQUIPMENT WORK FLOW CHART

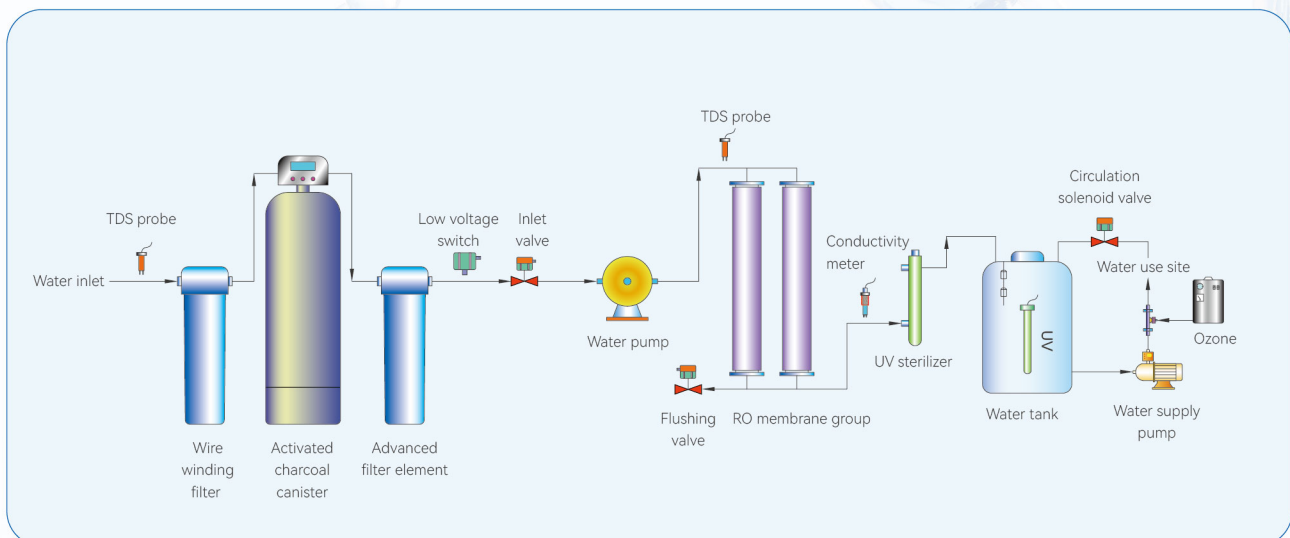

EQUIPMENT PARAMETER INFORMATION

EQUIPMENT PARAMETERS AND RELEVANT REQUIREMENTS	
Equipment model	YS-RO-150L/H
Water quality standards	WS 507-2016
Water output	150L/H
Quality of water production	
Microbial limit	≤10 CFU/100ml
Electrical conductivity μs/cm(25°C)	0.0050
Additional information	
Equipment size	54*56*148cm
Usage requirement	
Incoming water pressure	≥0.3MPa
Influent quality (TDS)	≤150ppm
Power supply	AC220V±10% 50HZ
Rated power	0.7kw
Scope of application	
Endoscope room disinfection and cleaning water	

EQUIPMENT CHARACTERISTICS AND ADVANTAGES



Artistic shape and appearance



Automatic start-stop



Renowned brand accessories at home and aboard



Easy installation and convenient replacement of consumables



Stable water production and quality



High water purity



Having independent intellectual property rights



IoT

YS-RO-200L/H



YS-RO-200L/H series medical pure water treatment system utilizes single-stage RO system.



The equipment of this model is equipped with an external water tank.




The water quality produced by the equipment of this model conforms to WS 507-2016 Regulation for Cleaning and Disinfection Technique of Flexible Endoscope. The equipment is measured by conductivity meter, and the conductivity is $\leq 15\mu\text{s}/\text{cm}$ (25°C).




The equipment utilizes multi-sterilization process of membrane module + overflow ultraviolet + immersion sterilization module + advanced oxidation + terminal filtration to ensure the safety of customer water.



The preprocessing of the equipment of this model adopts multiple filtration methods: The first-class 20-inch thick wire winding, second-class canned coconut shell activated carbon/softened resin (with timing automatic washing), and third class 20-inch thick precision filtration, applicable to different areas of water quality, satisfy multiple customer needs.

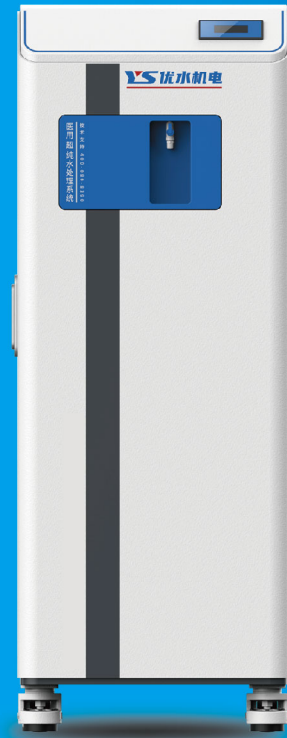

EQUIPMENT WORK FLOW CHART

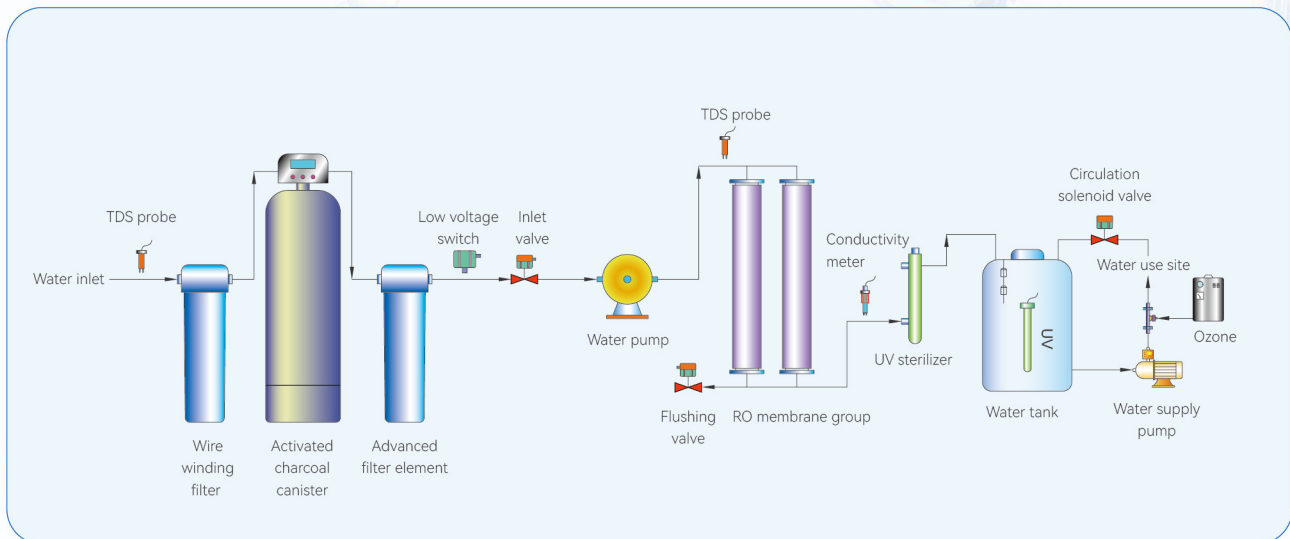

EQUIPMENT PARAMETER INFORMATION

EQUIPMENT PARAMETERS AND RELEVANT REQUIREMENTS	
Equipment model	YS-RO-200L/H
Water quality standards	WS 507-2016
Water output	200L/H
Quality of water production	
Microbial limit	≤10 CFU/100ml
Electrical conductivity μs/cm(25°C)	0.0050
Additional information	
Equipment size	54*56*148cm
Usage requirement	
Incoming water pressure	≥0.3MPa
Influent quality (TDS)	≤150ppm
Power supply	AC220V±10% 50HZ
Rated power	0.75kw
Scope of application	
Endoscope room disinfection and cleaning water	

EQUIPMENT CHARACTERISTICS AND ADVANTAGES



Artistic shape and appearance



Automatic start-stop



Renowned brand accessories at home and aboard



Easy installation and convenient replacement of consumables



Stable water production and quality



High water purity



Having independent intellectual property rights



IoT

YS-RO-(300/500)L/H



YS-RO-(300-500)L/H series medical pure water treatment system utilizes single-stage RO system.



The equipment of this model is equipped with an external water tank.




The water quality produced by the equipment of this model conforms to WS 507-2016 Regulation for Cleaning and Disinfection Technique of Flexible Endoscope. The equipment is measured by conductivity meter, and the conductivity is $\leq 15\mu\text{s}/\text{cm}$ (25°C).




The equipment utilizes multi-sterilization process of membrane module + overflow ultraviolet + immersion sterilization module + advanced oxidation + terminal filtration to ensure the safety of customer water.



The preprocessing of the equipment of this model adopts multiple filtration methods: The first-class 20-inch thick wire winding, second-class canned coconut shell activated carbon/softened resin (with timing automatic washing), and third class 20-inch thick precision filtration, applicable to different areas of water quality, satisfy multiple customer needs.

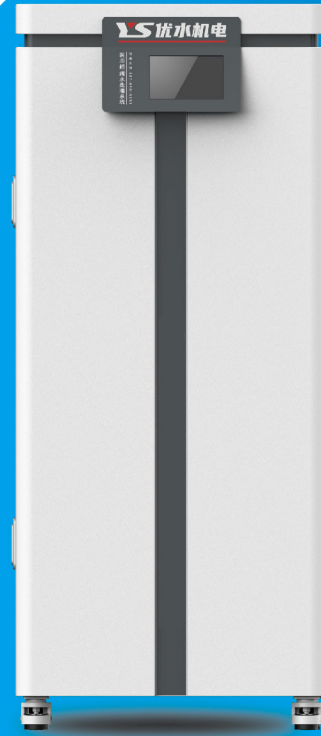

EQUIPMENT WORK FLOW CHART

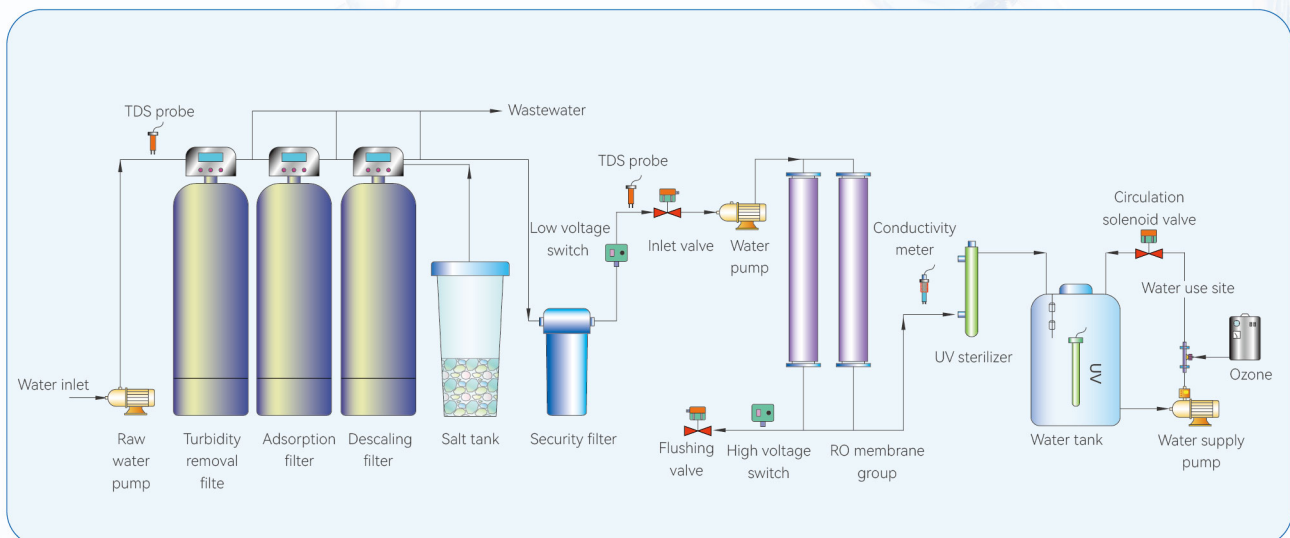

EQUIPMENT PARAMETER INFORMATION

EQUIPMENT PARAMETERS AND RELEVANT REQUIREMENTS	
Equipment model	YS-RO- (300/500) L/H
Water quality standards	WS 507-2016
Water output	(300/500)L/H
Quality of water production	
Microbial limit	≤10 CFU/100ml
Electrical conductivity μs/cm(25°C)	0.0050
Additional information	
Equipment size	72*86*170cm
Usage requirement	
Incoming water pressure	≥0.3MPa
Influent quality (TDS)	≤150ppm
Power supply	AC220V±10% 50HZ
Rated power	(1.35/1.5)kw
Scope of application	
Endoscope room disinfection and cleaning water	

EQUIPMENT CHARACTERISTICS AND ADVANTAGES



Artistic shape and appearance



Automatic start-stop



Renowned brand accessories at home and aboard



Easy installation and convenient replacement of consumables



Stable water production and quality



High water purity



Having independent intellectual property rights



IoT



First-class products
first-class brand
first-class service



Quality and ultra-pure
water online



Customer service
WeChat

Hefei Youshui Mechanical Electric Equipment Co., Ltd.

Address: Building 3B, 2nd Floor, YosiTech High-Tech Innovation
Industrial Park, Hefei High-Tech Development Zone

Tel: 0551-65655086

Service hotline: 400-0808-390